


MS Spectrum

Positive

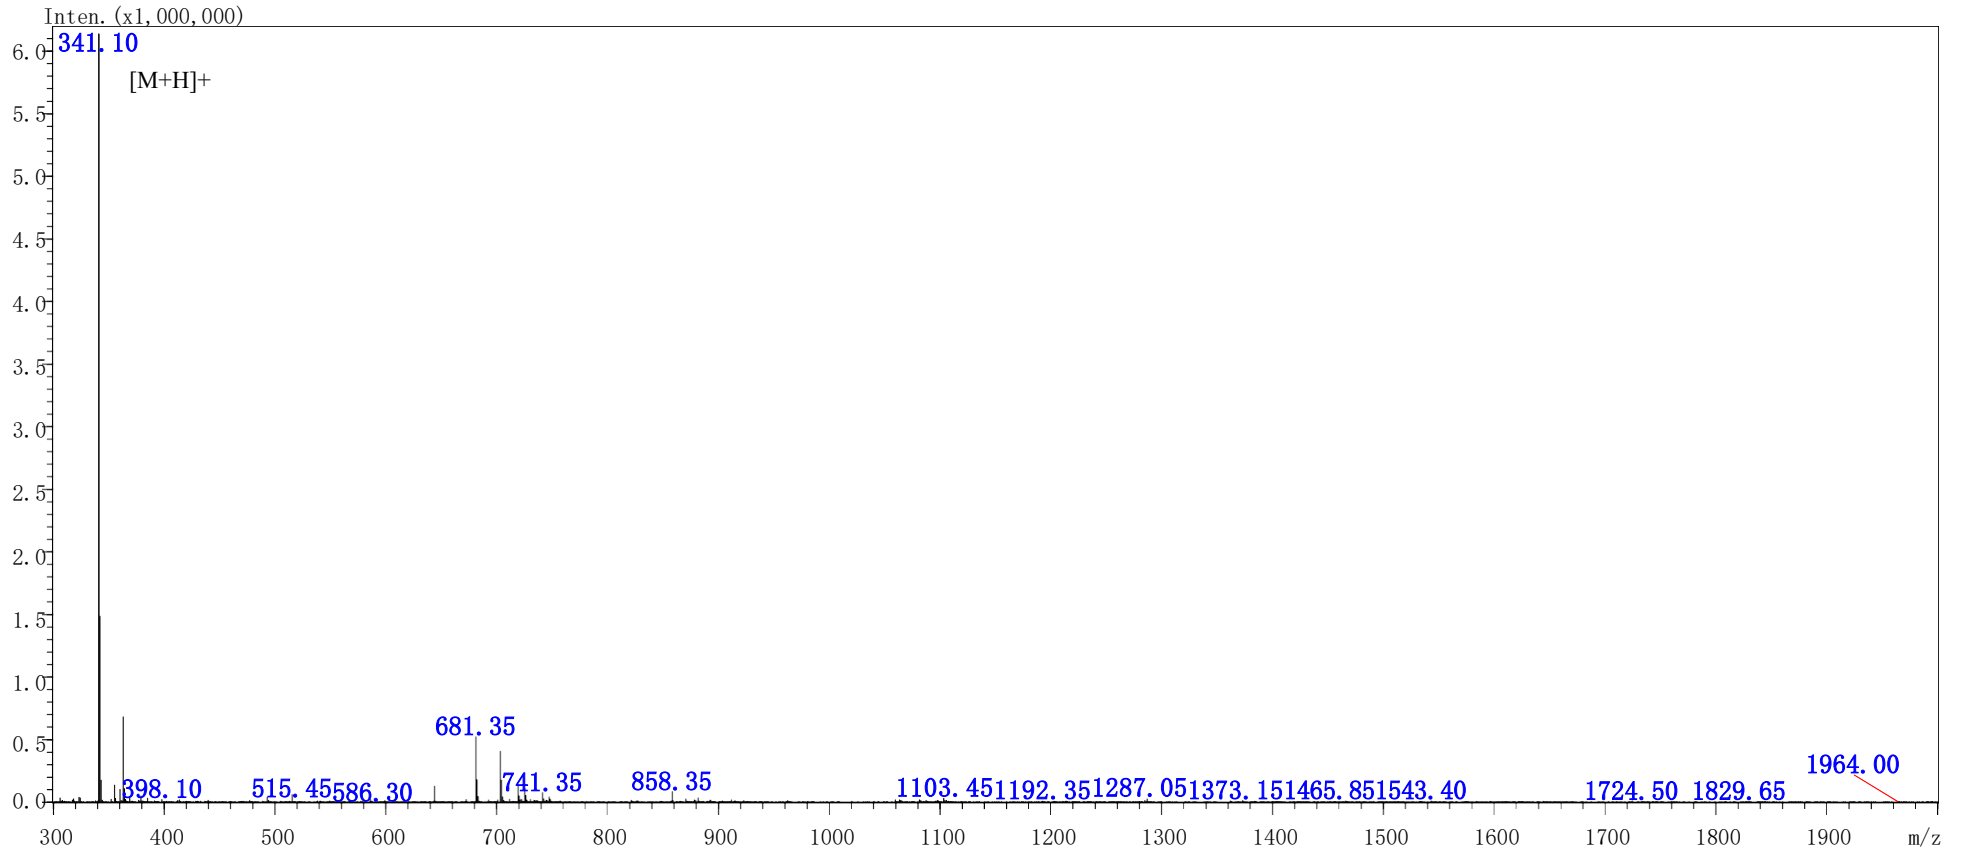

Acquiredby :Shen
DataAcquired :2023/5/9
Injection Volume :1
SampleName :Copper PeptideGK-3-Cu
Mw :340.37
LotNo. :P230314-LR549012

Probe :ESI
Nebulizer GasFlow :1.5L/min
CDL :-20.0v
CDLTemp :250°C
BlockTemp :400°C
Probebias :+4.5kv
Detector :1.2kv
T.Flow :0.2ml/min
B.conc :50%H2O/50%ACN